
User manual M3

Thermocouple type K, B, S, N, E, T, R, L, J



Technical features:

- red display from -19999...99999 digits (optional green, orange or blue display)
- minimal installation depth: 90 mm without plug-in terminal
- adjustment via factory default or directly on the sensor signal
- min/max-value recording
- display flashing at threshold exceedance / undercut
- Hold-function
- permanent min/max-value recording
- **volume measuring (totaliser)**
- mathematical functions like reciprocal value, square root, square, rounding
- programming interlock via access code
- protection class IP65 at the front
- plug-in screw terminal
- optional: 2 PhotoMos outputs
- optional: sensor supply or analog output
- optional: digital output
- accessories: pc-based configuration kit PM-TOOL incl. CD & USB adapter for devices without keypad, for a simple adjustment of standard devices

Identification

STANDARD-TYPES	ORDER NUMBER
Thermocouple	M3-7TR5A.040X.S70xD
Housing size: 48x24 mm	M3-7TR5A.040X.770xD

Options – breakdown of order code:

	M	3	7	T	R	5	B.	0	4	0	X.	7	7	2	x	D		
Standard type M line																		Dimension
																		<input type="checkbox"/> D physical unit
Installation depth																		Version
109 mm, incl. plug-in terminal																		<input type="checkbox"/> x internal version
Housing size																		Switching points
48x24x90 mm (BxHxD)																		<input type="checkbox"/> 0 no switching point
																		<input type="checkbox"/> 2 2 PhotoMos-outputs
Display type																		Protection class
Temperature																		<input type="checkbox"/> 1 without keypad, operation via PM-TOOL
Display colour																		<input type="checkbox"/> 7 IP65 / plug-in terminal
Blue																		Supply voltage
Green																		<input type="checkbox"/> 7 24 VDC galv. isolated
Red																		<input type="checkbox"/> S 85-265 VAC
Orange																		Measuring input
Number of digits																		<input type="checkbox"/> X Type K, B, S, N, E, T, R, L, J
5-digit																		Analog output
Digit height																		<input type="checkbox"/> 0 without
10 mm																		<input type="checkbox"/> X 0-10 VDC, 0/4-20 mA
Digital input																		Temperature devices
without																		<input type="checkbox"/> 4 Thermocouple
1 digital input																		

Please state physical unit by order.

Contents

1.	Brief description	2
2.	Assembly	2
3.	Electrical connection	3
4.	Functions and operation description	4
	4.1. Programming software PM-TOOL	5
5.	Setting up the device	6
	5.1. Switching on	6
	5.2. Standard parameterisation (flat operation level)	6
	Value assignment for triggering of the signal input	
	5.3. Programming interlock „RUN“	9
	Activation/Deactivation of the programming interlock or change into the professional level respectively back into the flat operation level	
	5.4. Extended parameterisation (professional operation level)	10
	5.4.1. Signal input parameter „INP“	10
	Value assignment for triggering of the signal input	
	5.4.2. General device parameter „FCT“	12
	Superior device functions like min/max permanent, brightness control, as well as the control of the keyboard configuration	
	5.4.3. Safety parameter „COD“	14
	Assignment of user and master code for locking or access to certain parameters like e.g. analog output and alarms, etc.	
	5.4.4. Analog output parameter „OUT“	15
	Analog output functions	
	5.4.5. Relay functions „REL“	17
	Parameter for the definition of the setpoints	
	5.4.6. Alarm parameter „AL1...AL4“	19
	Activator and dependencies of the alarms	
6.	Reset to factory settings	21
	Reset of the parameter to the factory default settings	
7.	Alarms / Relays	22
	Function principle of the switching outputs	
8.	Technical data	23
9.	Safety advices	25
10.	Error elimination	26

1. Brief description

The panel meter instrument **M3-3T** is a 5-digit device for Thermocouple and a visual threshold value monitoring via the display. The configuration happens via four keys at the front or by the optional PC software PM-TOOL. The integrated programming interlock prevents unrequested changes of parameters and can be unlocked again with an individual code. Optional available is one analog output for further evaluating in the unit.

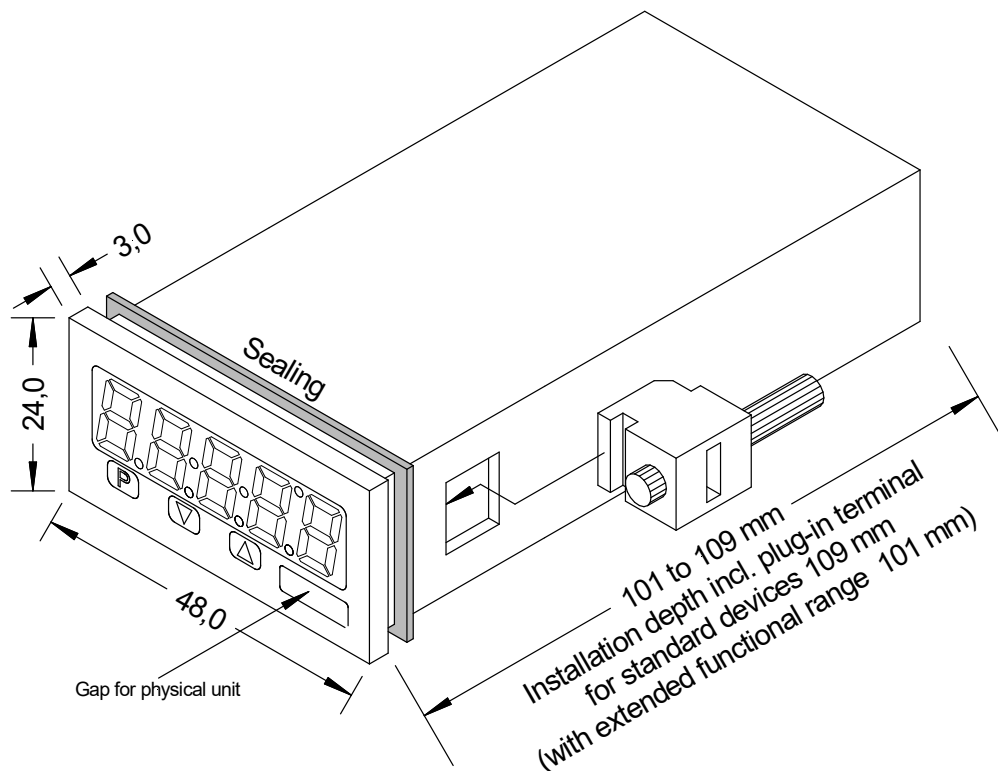
With help of the two galvanic isolated setpoints (optional), free adjustable limit values can be controlled and reported to a superior master display.

The electrical connection is done via plug-in terminals on the back side.

Selectable functions like e.g. the recall of the min/max-value, a direct threshold value regulation during operation mode, complete the modern device concept.

2. Assembly

Please read the *Safety advices* on page 25 before installation and keep this user manual for future reference.



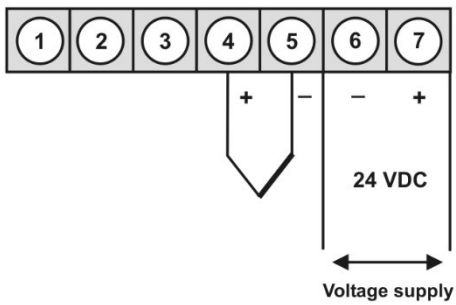
1. After removing the fixing elements, insert the device.
2. Check the seal to make sure it fits securely.
3. Click the fixing elements back into place and tighten the clamping screws by hand. Then use a screwdriver to tighten them another half a turn.

CAUTION! The torque should not exceed 0.1 Nm!

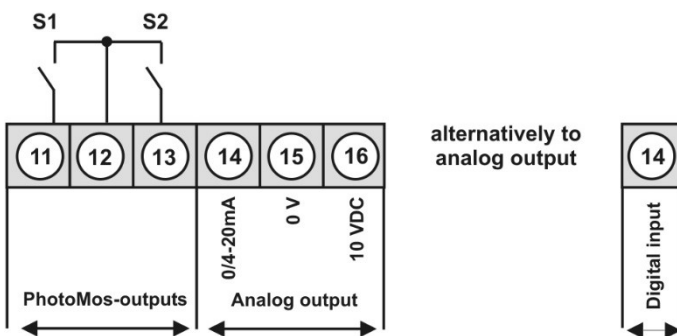
**Change signs of the physical unit before assembly via a channel at the side of the front!
The change can only be done from the outside before assembly!**

3. Electrical connection

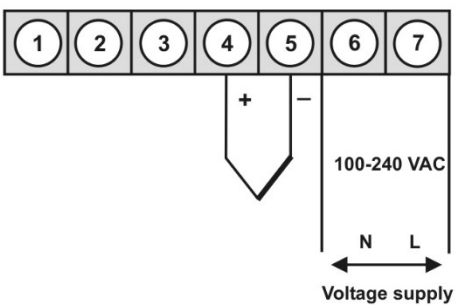
Type M3-7TR5A.040X.770xD
 supply of 24 VDC



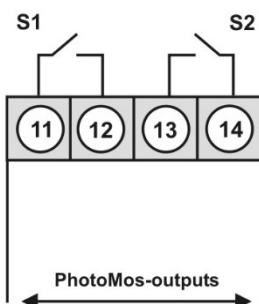
Options:



Type M3-7TR5A.040X.S70xD
 supply of 100-240 VAC



Options:



4. Function and operation description

Operation

The operation is divided into three different levels.

Menu level (delivery status)
















The menu level is for the standard settings of the device. Only menu items which are sufficient to set the device into operation are displayed. To get into the professional level, run through the menu level and parameterise "PROF" under menu item *RUN*.

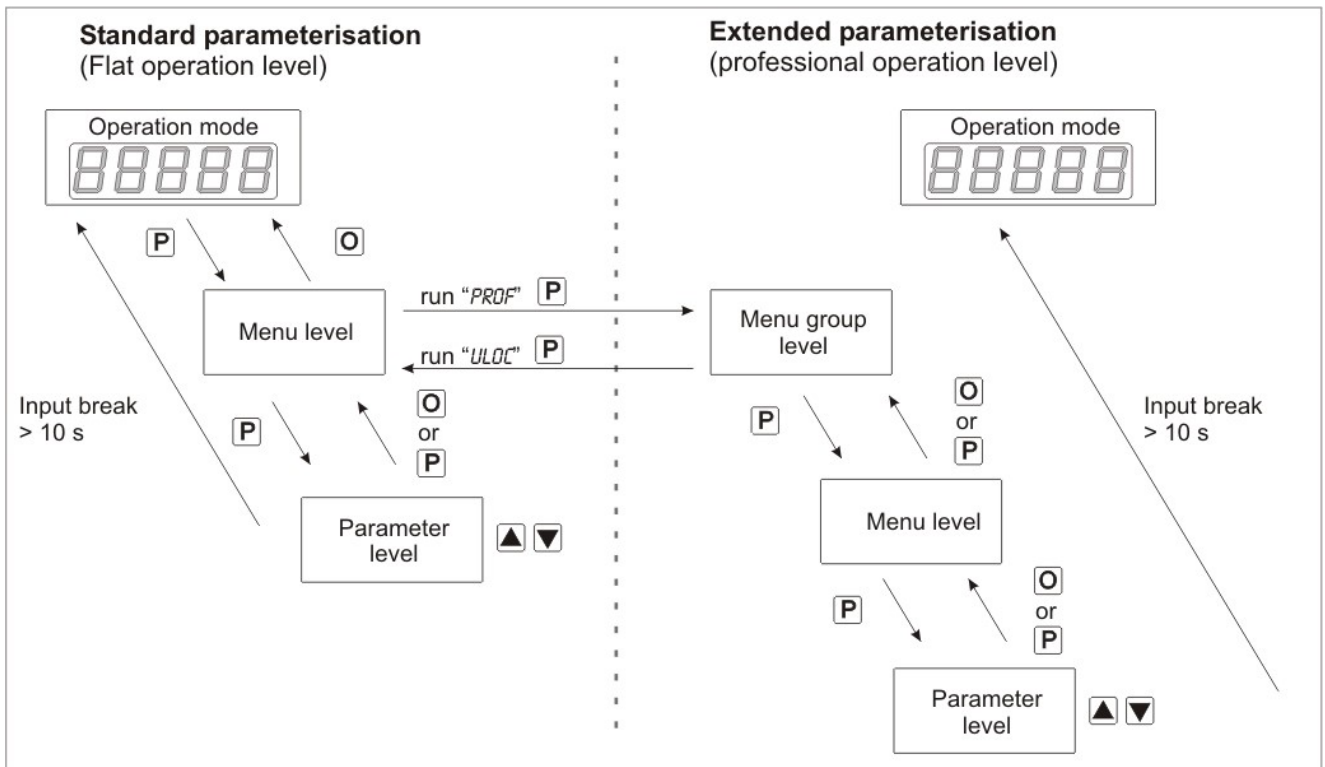
Menu group level (complete function volume)

Suited for complex applications as e.g. linkage of alarms, setpoint treatment, totaliser function etc. In this level function groups which allow an extended parameterisation of the standard settings are available. To leave the menu group level, run through this level and parameterise „ULOC„ under menu item *RUN*.

Parameterisation level:

Parameter deposited in the menu item can here be parameterised. Functions, that can be changed or adjusted, are always signalled by a flashing of the display. Settings that are made in the parameterisation level are confirmed with **[P]** and thus saved. Pressing the **[O]**-key („zero-key“) leads to a break-off of the value input and to a change into the menu level. All adjustments are saved automatically by the device and it changes into operating mode, if no further key operation is done within the next 10 seconds.

Level	Key	Description
Menu level		Change to parameterisation level and deposited values.
	 	Keys for up and down navigation in the menu level.
	 	Change into operation mode by pushing both navigation keys at the same time.
Parameterisation level		To confirm the changes made at the parameterization level.
	 	Adjustment of the value / the setting.
	 	Change into menu level or stop of the value input, by pushing both navigation keys at the same time.
Menu group level		Change to menu level
	 	Keys for up and down navigation in the menu group level.
	 	Change into operation mode or return into menu level, by pushing both navigation keys at the same time.

Function chart:**Underline:**

- P** Takeover
- O** Stop
- ▲** Value selection (+)
- ▼** Value selection (-)

4.1 Parameterisation software PM-TOOL:

Included in the delivery of the PM-TOOL are the software on CD and an USB-cable with device adapter. The connection happens via a 4-pole micromatch-plug on the back side of the device, to the PC-side the connection happens via an USB plug.

System requirements: PC incl. USB interface
Software: Windows XP, Windows VISTA

With this tool the device configuration can be generated, omitted and saved on the PC. The parameters can be changed via the easy to handle program surface, whereat the operating mode and the possible selection options can be preset by the program.

CAUTION!

During parameterisation with connected measuring signal, make sure that the measuring signal has no mass supply to the programming plug. The programming adapter is galvanic not isolated and directly connected with the PC. Via polarity of the input signal, a current can discharge via the adapter and destroy the device as well as other connected components!

5. Setting up the device

5.1. Switching on









Once the installation is complete, start the device by applying the voltage supply. Before, check once again that all electrical connections are correct.







Starting sequence






For 1 second during the switching-on process, the segment test (θ θ θ θ θ) is displayed followed by an indication of the software type and, after that, also for 1 second the software version. After the starting sequence, the device switches to operation/display mode.



5.2. Standard parameterisation: (Flat operation level)

To parameterise the display, press the **[P]**-key in operating mode for 1 second. The display then changes to the menu level with the first menu item *TYPE*.

Menu level	Parameterisation level
	<p>Selection of the input signal, <i>TYPE</i>: Default: <i>TYP.L</i></p> <p>  </p> <p>Available are 9 types of thermocouple as input options (L, J, K, B, S, N, E, T, R). Confirm the selection with [P] and the display switches back to menu level.</p>
	<p>Type of temperature metering, <i>UNIT</i>: Default: °C</p> <p>  </p> <p>The temperature can be displayed in °C or in °F. Confirm the selection with [P] and the display switches back to menu level.</p>
	<p>Setting the decimal point, <i>DOT</i>: Default: <i>0.0</i></p> <p>  </p> <p>The decimal point on the display and the physical unit can be changed with [▲] [▼]. If e.g. temperature measurement in °C is selected, then select between 0°C and 0.0°C in the parameterisation level. Confirm with [P], the display then switches back to the menu level again.</p>
	<p>Setting the measuring range start/offset value, <i>OFFS</i>: Default: <i>0.0</i></p> <p>  </p> <p>The value for the sensor calibration is selectable from the smallest to the highest digit with [▲] [▼] and confirmed with [P]. After the last digit the display switches back to the menu level again. The value calibration for a temperature measurement in °C can be adjusted between -20.0 and +20.0 and in °F between -36.0 and +36.0. If the type of the measurement is changed later, then the value is rounded.</p>

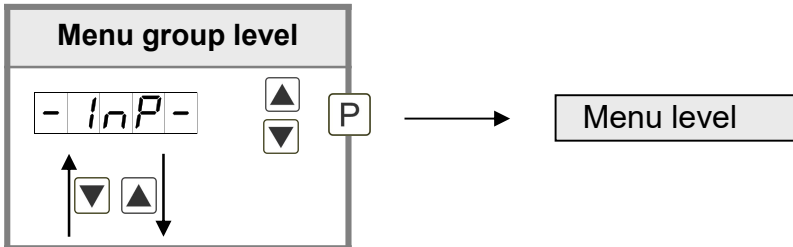
Menu level	Parameterisation level
	<p>Setting the display time, SEC: Default: 1.0</p> <p>SEC P 00.1 ▲ ▼ 00.9 then 0.10 ▲ ▼ 10.0 ▲ ▼ P</p> <p>The display time is set with [▲] [▼]. The display moves up in increments of 0.1 up to 1 second and in increments of 1.0 to 10.0 seconds. Confirm the selection by pressing the [P] button. The display then switches back to the menu level again.</p>
	<p>Selection of analog output, OUT.RA: Default: 4-20</p> <p>Out.RA P 0-10 ▲ ▼ 0-20 ▲ ▼ 4-20 ▲ ▼ P</p> <p>Available are 3 output signals: 0-10 VDC, 0-20 mA and 4-20 mA. With this function, the demanded signal is selected.</p>
	<p>Setting up the final value of the analog output, OUT.EN: Default: 850.00</p> <p>Out.EN P 8 P 8 P 8 P 8 P 8 ▲ ▼ P</p> <p>The final value is adjusted from the smallest digit to the highest digit with [▲] [▼] and digit by digit confirmed with [P]. A minus sign can only be parameterised on the leftmost digit. After the last digit, the device changes back into menu level.</p>
	<p>Setting up the initial value of the analog output, OUT.OF: Default: -200.0</p> <p>Out.OF P 8 P 8 P 8 P 8 P 8 ▲ ▼ P</p> <p>The initial value is adjusted from the smallest digit to the highest digit with [▲] [▼] and digit by digit confirmed with [P]. A minus sign can only be parameterised on the leftmost digit. After the last digit, the device changes back into menu level.</p>
	<p>Threshold values / limits, LI-1: Default: 200.0</p> <p>LI-1 P 0 P 0 P 0 P 0 P 0 ▲ ▼ P</p> <p>This value defines the threshold, that activates/deactivates an alarm.</p>
	<p>Hysteresis for limit values, HY-1: Default: 0.0</p> <p>HY-1 P 0 P 0 P 0 P 0 P 0 ▲ ▼ P</p> <p>The delayed reaction of the alarm is the difference to the threshold value, which is defined by the hysteresis.</p>

Menu level	Parameterisation level
	<p>Function for threshold value undercut / exceedance, FU-1: Default: <i>HIGH</i></p> <p>FU-1 [P] HIGH [▲] [▼] LOW [▲] [▼] [P]</p> <p>A limit value undercut is selected with <i>LOW</i> (for LOW = lower limit value), a limit value exceedance with <i>HIGH</i> (for HIGH = higher limit value). If e.g. limit value 1 is on a threshold level of 100 and allocated with function <i>HIGH</i>, an alarm is activated by reaching the threshold level. If the threshold value was allocated to <i>LOW</i>, an alarm will be activated by undercutting the threshold value, as long as the hysteresis is zero.</p>
	<p>Threshold values / limits, LI-2: Default: <i>300.0</i></p> <p>LI-2 [P] 0 [P] 0 [P] 0 [P] 0 [P] 0 [▲] [▼] [P]</p> <p>This value defines the threshold, that activates/deactivates an alarm.</p>
	<p>Hysteresis for threshold values, HY-2: Default: <i>0.0</i></p> <p>HY-2 [P] 0 [P] 0 [P] 0 [P] 0 [P] 0 [▲] [▼] [P]</p> <p>The delayed reaction of the alarm is the difference to the threshold value, which is defined by the hysteresis.</p>
	<p>Function if display falls below / exceeds limit value, FU-2: Default: <i>HIGH</i></p> <p>FU-2 [P] HIGH [▲] [▼] LOW [▲] [▼] [P]</p> <p>A limit value undercut is selected with <i>LOW</i> (for LOW = lower limit value), a limit value exceedance with <i>HIGH</i> (for HIGH = higher limit value). If e.g. limit value 1 is on a threshold level of 100 and allocated with function <i>HIGH</i>, an alarm is activated by reaching the threshold level. If the threshold value was allocated to <i>LOW</i>, an alarm will be activated by undercutting the threshold value, as long as the hysteresis is zero.</p>
	<p>User code (4-digit number-combination, free available), U.CODE: Default: <i>0000</i></p> <p>U.CODE [P] 0 [P] 0 [P] 0 [P] 0 [▲] [▼] [P]</p> <p>If this code was set (>0000), all parameters are locked for the user, if <i>LOC</i> has been selected before under menu item <i>RUN</i>. By pressing [P] for 3 seconds in operation mode, the display shows <i>CODE</i>. The <i>U.CODE</i> needs to be entered to get to the reduced number of parameter sets. The code has to be entered before each parameterisation, until the <i>R.CODE</i> (Master code) unlocks all parameters again.</p>








Menu level	Parameterisation level
	<p>Master code (4-digit number-combination, free available), <i>R.CODE</i>: Default: 1234</p> <p><i>R.CodE</i> [P] 8 [P] 8 [P] 8 [P] 8 [▲] [▼] [P]</p> <p>All parameters can be released with this code, after <i>LOC</i> has been activated under menu item <i>RUN</i>. By pressing [P] for 3 seconds in operation mode, the display shows <i>CODE</i> and enables the user to reach all parameters by entering the <i>R.CODE</i>. Under <i>RUN</i> the parameterisation can be activated permanently by selecting <i>ULOC</i> or <i>PROF</i>, thus at an anew pushing of [P] in operation mode, the code needs not to be entered again.</p>
<h3>5.3. Programming interlock „<i>RUN</i>“</h3>	
	<p>Activation / deactivation of the programming lock or completion of the standard parameterization with change into menu group level (complete function range), <i>RUN</i>: Default: <i>ULOC</i></p> <p><i>run</i> [P] <i>ULOC</i> [▲] [▼] <i>LOC</i> [▲] [▼] <i>PROF</i> [▲] [▼] [P]</p> <p>Choose between the deactivated key lock <i>ULOC</i> (works setting) and the activated key lock <i>LOC</i>, or the change into the menu group level <i>PROF</i>. With the navigation keys [▲] [▼]. Confirm the selection with [P]. After this, the display confirms the settings with "- - - -", and automatically switches to operating mode. If <i>LOC</i> was selected, the keyboard is locked. To get back into the menu level, press [P] for 3 seconds in operating mode. Now enter the <i>CODE</i> (works setting 1 2 3 4) that appears using [▲] [▼] plus [P] to unlock the keyboard. <i>FAIL</i> appears if the input is wrong. To parameterize further functions <i>PROF</i> needs to be set. The device confirms this setting with „- - - -“, and changes automatically in operation mode. By pressing [P] for approx. 3 seconds in operation mode, the first menu group <i>INP</i> is shown in the display and thus confirms the change into the extended parameterisation. It stays activated as long as <i>ULOC</i> or <i>LOC</i> is entered in menu group <i>RUN</i>.</p>

5.4. Extended parameterisation (Professional operation level)

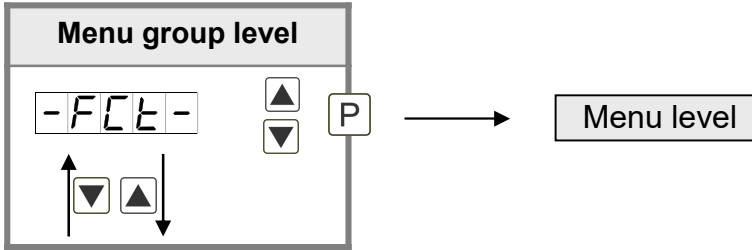
5.4.1. Signal input parameters






Menu level	Parameterisation level
	<p>Selection of the input signal, TYPE: Default: <i>TYPE.L</i></p> <p>Available are 9 types of thermocouple as input options (L, J, K, B, S, N, E, T, R). Confirm the selection with [P] and the display switches back to menu level.</p>
	<p>Type of temperature metering UNIT: Default: °C</p> <p>The temperature can be displayed in °C or in °F. Confirm the selection with [P] and the display switches back to menu level.</p>
	<p>Setting the decimal point, DOT: Default: 0.0</p> <p>The decimal point on the display and the physical unit can be changed with [▲][▼]. If e.g. temperature measurement in °C is selected, then select between 0°C and 0.0°C in the parameterisation level. Confirm with [P], the display then switches back to the menu level again.</p>
	<p>Setting the measuring range start/offset value, OFFS: Default: 0.0</p> <p>The value for the sensor calibration is selectable from the smallest to the highest digit with [▲][▼] and confirmed with [P]. After the last digit the display switches back to the menu level again. The value calibration for a temperature measurement in °C can be adjusted between -20.0 and +20.0 and in °F between -36.0 and +36.0. If the type of the measurement is changed later, then the value is rounded.</p>

Menu level	Parameterisation level
	<p>Setting the display time, SEC: Default: 1.0</p>  <p>The display time is set with [▲] [▼]. The display moves up in increments of 0.1 up to 1 second and in increments of 1.0 to 10.0 seconds. Confirm the selection by pressing the [P] button. The display then switches back to the menu level again.</p>
	<p>Display underflow, DI.UND: Default: -19999</p>  <p>With this function the device undercut (____) can be defined on a definite value.</p>
	<p>Display overflow, DI.OUE: Default: 99999</p>  <p>With this function the display overflow (-----) can be defined on a definite value.</p>
	<p>Back to menu group level, RET:</p> <p>With [P] the selection is confirmed and the device changes into menu group level „-IMP-“.</p>

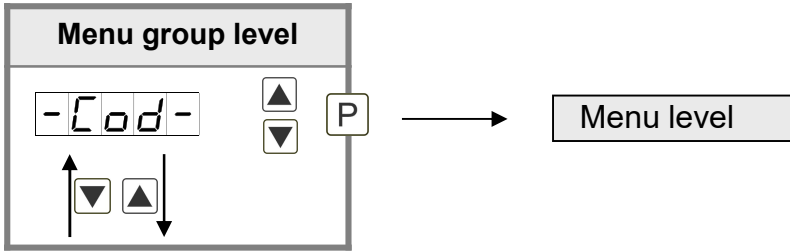
5.4.2. General device parameters




Menu level	Parameterisation level
	<p>Display time, <i>DISEC</i>: Default: 01.0</p> <p> then </p> <p>The display is set up with [▲] [▼]. Thereby it switches until 1 second in increments of 0.1 seconds and until 10.0 seconds in increments of 1.0. With [P] the selection is confirmed and the device changes into menu level.</p>
	<p>Rounding of display values, <i>ROUND</i>: Default: 00001</p> <p> </p> <p>This function is for instable display values, where the display value is changed in increments of 1, 5, 10 or 50. This does not affect the resolution of the optional outputs. With [P] the selection is confirmed and the device changes into menu level.</p>
	<p>Display, <i>DISPL</i>: Default: ACTUA</p> <p> </p> <p>With this function the current measurand, min/max-value or the process-controlled Hold-value can be allocated to the display. With [P] the selection is confirmed and the device changes into menu level.</p>
	<p>Display flashing, <i>FLASH</i>: Default: NO</p> <p> </p> <p>A display flashing can be added as additional alarm function either to single or to a combination of off-limit condition. With <i>NO</i>, no flashing is allocated.</p>

Menu level	Parameterisation level
 <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 10px;">EASE</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 10px;">P</div>	<p>Assignment (deposit) of key functions, TAST: Default: <i>NO</i></p> <div style="display: flex; justify-content: space-around; align-items: flex-start; margin-bottom: 10px;"> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">EHTR</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">LI.12</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">LI.34</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">EHTRE</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> </div> <div style="display: flex; justify-content: space-around; align-items: flex-start;"> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">ACTUA</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">no</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 10px;">P</div> </div> <p>For the operation mode, special functions can be deposited on the navigation keys [▲] [▼], in particular this function is made for devices in housing size 48x24mm which do not have a 4th key ([O]-key). If the min/max-memory is activated with <i>EHTR</i>, all measured min/max-values are saved during operation and can be recalled via the navigation keys. The values get lost by restart of the device. If the threshold value correction <i>LI.12</i> or <i>LI.34</i> is chosen, the values of the threshold can be changed during operation without disturbing the operating procedure. If <i>NO</i> is selected, the navigation keys are without function in the operation mode.</p>
 <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 10px;">DIGIN</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 10px;">P</div>	<p>Special function digital input, DIG.IN: Default: <i>NO</i></p> <div style="display: flex; justify-content: space-around; align-items: flex-start; margin-bottom: 10px;"> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">EHTRE</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">ACTUA</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">HOLD</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> </div> <div style="display: flex; justify-content: space-around; align-items: flex-start;"> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">AL-1 ...</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">AL-4</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 5px;">no</div> <div style="text-align: center; margin: 0 5px;">▲ ▼</div> <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 10px;">P</div> </div> <p>For operating mode, special functions can be realised via the digital input. This function is actuated by a voltage signal on the terminal of the digital input. With <i>TARA</i> the device is tared to zero and saved permanently as offset. The display acknowledges this with <i>00000</i> in the display. <i>SET.TA</i> switches into the offset value and can be changed via the navigation keys. Via <i>TOTAL</i> the current value of the totaliser can be displayed for approx. 7 seconds, after this the device switches back on the parameterised display value. If <i>TOT.RE</i> is deposited, the totaliser can be set back by switching on the digital input, the device acknowledges this with <i>00000</i> in the display. <i>EHT.RE</i> deletes the min/max-memory. If <i>HOLD</i> has been selected, the moment can be hold constant by pressing the [O]-key, and is updated by releasing the key. Advice: <i>HOLD</i> is activated only, if <i>HOLD</i> was selected under parameter <i>DISPL</i>. <i>ACTUA</i> shows the measurand for approx. 7 seconds, after this the device switches back on the parameterised display value. At <i>AL-1...AL-4</i>, an output can be set and therewith e.g. a setpoint adjustment can be done. If <i>NO</i> is selected, the [O]-key is without any function in the operation mode.</p>
 <div style="border: 1px solid black; padding: 2px; display: inline-block; margin-right: 10px;">RET</div>	<p>Back to menu group level, RET:</p> <p>With [P] the selection is confirmed and the device changes into menu group level „-FCT-“.</p>

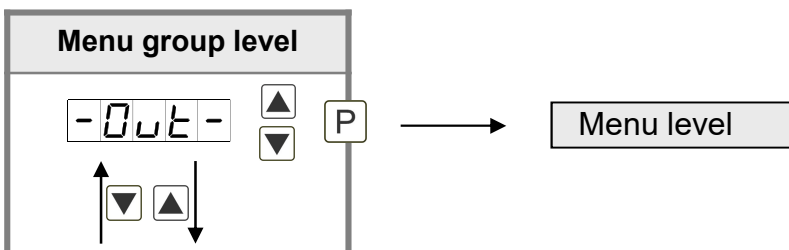
5.4.3. Safety parameters












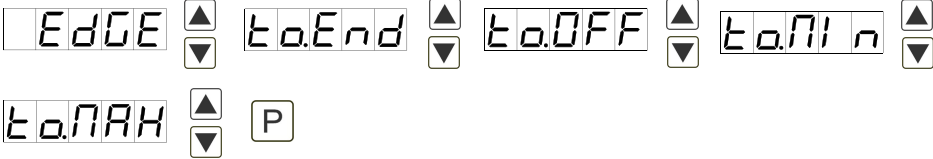

Menu level	Parameterisation level
	<p>User code <i>U.CODE</i>: Default: 0000</p> <p><i>U.CoDE</i> P 0 P 0 P 0 P 0 ▲ P ▼</p> <p>Via this code, reduced sets of parameters can be released. A change of the <i>U.CODE</i> can be done via the correct input of the <i>R.CODE</i> (master code).</p>
	<p>Master code, <i>R.CODE</i>: Default: 1234</p> <p><i>R.CoDE</i> P 1 P 2 P 3 P 4 ▲ P ▼</p> <p>By entering <i>R.CODE</i> the device will be unlocked and all parameters are released.</p>
	<p>Release/lock analog output parameters, <i>OUT.LE</i>: Default: ALL</p> <p><i>OutLE</i> P no ▲ EN-OF ▼ <i>Out.EO</i> ▲ ▼ ALL P</p> <p>Analog output parameters can be locked or released for the user:</p> <ul style="list-style-type: none"> - <i>EN-OF</i>: the initial or final value can be changed in operation mode - <i>OUT.EO</i>: the output signal can be changed from e.g. 0-20 mA to 4-20 mA or 0-10 VDC - <i>ALL</i>: analog output parameters are released - <i>NO</i>: all analog output parameters are locked
	<p>Release/lock alarm parameters, <i>AL.LEU</i>: Default: ALL</p> <p><i>ALLEU</i> P no ▲ LIMIT ▼ ALRM.L ▲ ▼ ALL P</p> <p>This parameter describes the user release/user lock of the alarm:</p> <ul style="list-style-type: none"> - <i>LIMIT</i>: here only the range of value of the threshold values 1-4 can be changed - <i>ALRM.L</i>: here the range of value and the alarm trigger can be changed - <i>ALL</i>: all alarm parameters are released - <i>NO</i>: all alarm parameters are locked

Menu level	Parameterisation level
	<p>Back to menu group level, <i>RET</i>:</p> <p>With [P] the selection is confirmed and the device changes into menu group level „-000-“.</p>

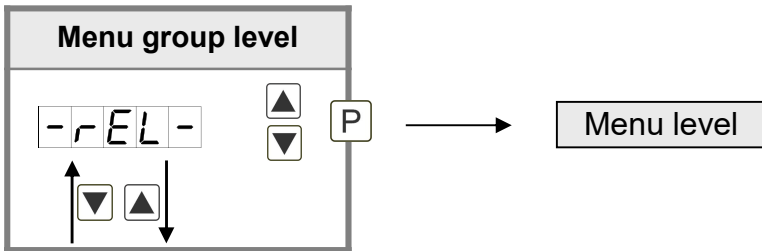
5.4.4. Analog output parameters for analog output






Menu level	Parameterisation level
	<p>Selection reference of analog output, <i>OUTPT</i>: Default: <i>ACTUA</i></p> <p>  </p> <p>The analog output signal can refer to different functions, in detail this are the current measuring value, min-value or max-value. If <i>HOLD</i> is selected the signal of the analog output will be hold and processed just after deactivation of <i>HOLD</i>. With [P] the selection is confirmed and the device changes into menu level.</p>
	<p>Selection analog output, <i>OUT.RA</i>: Default: 4-20</p> <p>  </p> <p>Available are 3 output signals: 0-10 VDC, 0-20 mA and 4-20 mA. With this function the demanded signal can be selected.</p>
	<p>Setting up the final value of the analog output, <i>OUT.EM</i>: Default: 10000</p> <p>  </p> <p>The final value can be adjusted from the smallest to the highest digit with [▲] [▼]. Confirm each digit with [P]. A minus sign can only be parameterized on the leftmost digit. After the last digit, the display switches back to the menu level.</p>



Menu level	Parameterisation level
	<p>Setting up the initial value of the analog output, <i>OUT.OF</i>: Default: 00000</p>  <p>The initial value can be adjusted from the smallest to the highest digit with [▲] [▼]. Confirm each digit with [P]. A minus sign can only be parameterized on the leftmost digit. After the last digit, the display switches back to the menu level.</p>
	<p>Overflow behaviour, <i>O.FLOW</i>: Default: <i>EDGE</i></p>  <p>To recognise and evaluate faulty signals, e.g. by a controller, the overflow behaviour of the analog output can be defined. As overflow can be seen either <i>EDGE</i>, that means the analog output runs on the set limits e.g. 4 and 20 mA, or <i>TO.OFF</i> (input value smaller than initial value, analog output switches on e.g. 4 mA), <i>TO.END</i> (higher than final value, analog output switches on e.g. 20 mA). If <i>TO.MIN</i> or <i>TO.MAX</i> is set, the analog output switches on the least significant or leftmost possible binary value. This means that values of e.g. 0 mA, 0 VDC or values higher than 20 mA or 10 VDC can be reached. With [P] the selection is confirmed and the device changes into menu level.</p>
	<p>Back to menu group level, <i>RET</i>:</p> <p>With [P] the selection is confirmed and the device changes into menu group level „-OUT-“.</p>

5.4.5. Relay functions

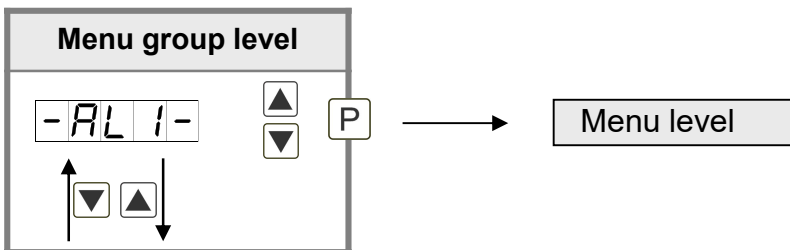




Menu level	Parameterisation level												
	<p>Alarm relay 1, REL-1: Default: <i>AL-1</i></p> <p> </p> <p>Each setpoint (optional) can be linked up via 4 alarms (by default). This can either be inserted at activated alarms <i>AL-1/4</i> or deactivated alarms <i>ALN1/4</i>. If <i>LOGIC</i> was selected, logical links are available in the menu level <i>LOG-1</i> and <i>COM-1</i>. Access to these two menu levels is via <i>LOGIC</i>, at all other selected functions, these two parameters are overlapped. Via <i>ON/OFF</i> the setpoints can be activated/deactivated, in this case the output and the setpoint display are set/not set on the front of the device. With [P] the selection is confirmed and the device changes into menu level.</p>												
	<p>Logic relay 1, LOG-1 Default: <i>OR</i></p> <p></p> <p>The switching behaviour of the relay is defined via a logic link, the following schema describes these functions with inclusion of <i>AL-1</i> and <i>AL-2</i>:</p> <table border="1"> <tbody> <tr> <td></td> <td>$A1 \vee A2$</td> <td>As soon as a selected alarm is activated, the relay operates. Equates to operating current principle.</td> </tr> <tr> <td></td> <td>$\overline{A1 \vee A2} = \overline{A1} \wedge \overline{A2}$</td> <td>The relay operates only, if no selected alarm is active. Equates to quiescent current principle.</td> </tr> <tr> <td></td> <td>$A1 \wedge A2$</td> <td>The relay operates only, if all selected alarms are active.</td> </tr> <tr> <td></td> <td>$\overline{A1 \wedge A2} = \overline{A1} \vee \overline{A2}$</td> <td>As soon as a selected alarm is not activated, the relay operates.</td> </tr> </tbody> </table> <p>With [P] the selection is confirmed and the device changes into menu level.</p>		$A1 \vee A2$	As soon as a selected alarm is activated, the relay operates. Equates to operating current principle.		$\overline{A1 \vee A2} = \overline{A1} \wedge \overline{A2}$	The relay operates only, if no selected alarm is active. Equates to quiescent current principle.		$A1 \wedge A2$	The relay operates only, if all selected alarms are active.		$\overline{A1 \wedge A2} = \overline{A1} \vee \overline{A2}$	As soon as a selected alarm is not activated, the relay operates.
	$A1 \vee A2$	As soon as a selected alarm is activated, the relay operates. Equates to operating current principle.											
	$\overline{A1 \vee A2} = \overline{A1} \wedge \overline{A2}$	The relay operates only, if no selected alarm is active. Equates to quiescent current principle.											
	$A1 \wedge A2$	The relay operates only, if all selected alarms are active.											
	$\overline{A1 \wedge A2} = \overline{A1} \vee \overline{A2}$	As soon as a selected alarm is not activated, the relay operates.											






Menu level	Parameterisation level													
	<p>Alarms for relay 1, COM-1: Default: <i>A.1</i></p> <p>COM-1 [P] A.1 [▲] [▼] A.2 [▲] [▼] ... A.1234 [▲] [▼] [P]</p>	<p>The allocation of the alarms to relay 1 happens via this parameter, one alarm or a group of alarms can be chosen. With [P] the selection is confirmed and the device changes into menu level.</p>												
	<p>Alarm relay 2, REL-2: Default: <i>AL-2</i></p> <p>REL-2 [P] AL-5 ... AL-8 [▲] [▼] AL-n5 ... AL-n8 [▲] [▼]</p> <p>LOGIC [▲] [▼] OFF [▲] [▼] On [▲] [▼] [P]</p>	<p>Each setpoint (optional) can be linked up via 4 alarms (by default). This can either be inserted at activated alarms <i>AL-1/4</i> or deactivated alarms <i>ALN1/4</i>. If <i>LOGIC</i> was selected, logical links are available in the menu level <i>LOG-1</i> and <i>COM-1</i>. Access to these two menu levels is via <i>LOGIC</i>, at all other selected functions, these two parameters are over-leaped. Via <i>ON/OFF</i> the setpoints can be activated/deactivated, in this case the output and the setpoint display are set/not set on the front of the device. With [P] the selection is confirmed and the device changes into menu level.</p>												
	<p>Logic relay 2, LOG-2: Default: <i>OR</i></p> <p>LOG-2 [P] or [▲] [▼] nor [▲] [▼] And [▲] [▼] nAnd [▲] [▼] [P]</p>	<p>The switching behaviour of the relay is defined via a logic link, the following schema describes these functions with inclusion of <i>AL-1</i> and <i>AL-2</i>.</p> <table border="1" data-bbox="336 1496 1498 1892"> <tbody> <tr> <td data-bbox="336 1496 523 1624"> <p>or</p> </td> <td data-bbox="523 1496 821 1624"> <p>$A1 \vee A2$</p> </td> <td data-bbox="821 1496 1498 1624"> <p>As soon as a selected alarm is activated, the relay operates. Equates to operating current principle.</p> </td> </tr> <tr> <td data-bbox="336 1624 523 1713"> <p>nor</p> </td> <td data-bbox="523 1624 821 1713"> <p>$\overline{A1 \vee A2} = \overline{A1} \wedge \overline{A2}$</p> </td> <td data-bbox="821 1624 1498 1713"> <p>The relay operates only, if no selected alarm is active. Equates to quiescent current principle.</p> </td> </tr> <tr> <td data-bbox="336 1713 523 1803"> <p>And</p> </td> <td data-bbox="523 1713 821 1803"> <p>$A1 \wedge A2$</p> </td> <td data-bbox="821 1713 1498 1803"> <p>The relay operates only, if all selected alarms are active.</p> </td> </tr> <tr> <td data-bbox="336 1803 523 1892"> <p>nAnd</p> </td> <td data-bbox="523 1803 821 1892"> <p>$\overline{A1 \wedge A2} = \overline{A1} \vee \overline{A2}$</p> </td> <td data-bbox="821 1803 1498 1892"> <p>As soon as a selected alarm is not activated, the relay operates.</p> </td> </tr> </tbody> </table> <p>With [P] the selection is confirmed and the device changes into menu level.</p>	<p>or</p>	<p>$A1 \vee A2$</p>	<p>As soon as a selected alarm is activated, the relay operates. Equates to operating current principle.</p>	<p>nor</p>	<p>$\overline{A1 \vee A2} = \overline{A1} \wedge \overline{A2}$</p>	<p>The relay operates only, if no selected alarm is active. Equates to quiescent current principle.</p>	<p>And</p>	<p>$A1 \wedge A2$</p>	<p>The relay operates only, if all selected alarms are active.</p>	<p>nAnd</p>	<p>$\overline{A1 \wedge A2} = \overline{A1} \vee \overline{A2}$</p>	<p>As soon as a selected alarm is not activated, the relay operates.</p>
<p>or</p>	<p>$A1 \vee A2$</p>	<p>As soon as a selected alarm is activated, the relay operates. Equates to operating current principle.</p>												
<p>nor</p>	<p>$\overline{A1 \vee A2} = \overline{A1} \wedge \overline{A2}$</p>	<p>The relay operates only, if no selected alarm is active. Equates to quiescent current principle.</p>												
<p>And</p>	<p>$A1 \wedge A2$</p>	<p>The relay operates only, if all selected alarms are active.</p>												
<p>nAnd</p>	<p>$\overline{A1 \wedge A2} = \overline{A1} \vee \overline{A2}$</p>	<p>As soon as a selected alarm is not activated, the relay operates.</p>												

Menu level	Parameterisation level
	<p>Alarms for relay 2, COM-2: Default: <i>A.2</i></p> <p>COM-2 [P] A.1 [▲] [▼] A.2 [▲] [▼] A.1234 [▲] [▼] [P]</p> <p>The allocation of the alarms to relay 5 happens via this parameter, one alarm or a group of alarms can be chosen. With [P] the selection is confirmed and the device changes into menu level.</p>
	<p>Back to menu group level, RET:</p> <p>RET [P]</p> <p>With [P] the selection is confirmed and the device changes into menu group level „-REL-“.</p>

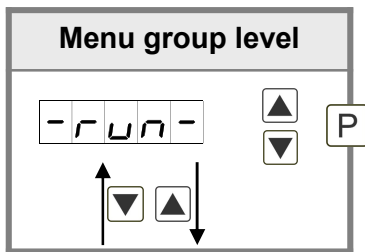
5.4.6. Alarm parameter



Menu level	Parameterisation level
	<p>Dependency alarm 1, ALRM.1: Default: <i>ACTUA</i></p> <p>ALRM.1 [P] ActUA [▲] [▼] MinUA [▲] [▼] MaxUA [▲] [▼] Hold [▲] [▼] EHTEr [▲] [▼] [P]</p> <p>The dependency of alarm 1 can be related to special functions, in detail these are the current measurand, the min-value or the max-value. If <i>HOLD</i> is selected, then the alarm is hold and processed just after deactivation of <i>HOLD</i>. <i>EHTER</i> causes the dependency by an external signal via the digital input. With [P] the selection is confirmed and the device changes into menu level.</p>
	<p>Threshold values / limit values, LI-1: Default: <i>200.0</i></p> <p>LI-1 [P] 0 [P] 0 [P] 0 [P] 0 [P] 0 [▲] [▼] [P]</p> <p>The limit value defines the threshold, that activates/deactivates an alarm.</p>

Menu level	Parameterisation level
	<p>Hysteresis for threshold values, <i>HY-1</i>: Default: <i>0.0</i></p> <p><i>HY-1</i> [P] 0 [P] 0 [P] 0 [P] 0 [P] 0 [P] 0 [P]</p> <p>The delayed reaction of the alarm is the difference to the threshold value, which is defined by the hysteresis.</p>
	<p>Function for threshold value undercut / exceedance, <i>FU-1</i>: Default: <i>HIGH</i></p> <p><i>FU-1</i> [P] <i>HIGH</i> [▲] [▼] <i>LOW</i> [▲] [▼] [P]</p> <p>A limit value undercut is selected with <i>LOW</i> (for LOW = lower limit value), a limit value exceedance with <i>HIGH</i> (for HIGH = higher limit value). If e.g. limit value 1 is on a threshold level of 100 and allocated with function <i>HIGH</i>, an alarm is activated by reaching the threshold level. If the threshold value was allocated to <i>LOW</i>, an alarm will be activated by undercutting the threshold value, as long as the hysteresis is zero.</p>
	<p>Switching-on delay, <i>TON-1</i>: Default: <i>000</i></p> <p><i>TON-1</i> [P] 0 [P] 0 [P] 0 [P] 0 [P] 0 [P] 0 [P]</p> <p>Preset a delayed switching-on of 0-100 seconds for limit value 1.</p>
	<p>Switching-off delay, <i>TOF-1</i>: Default: <i>000</i></p> <p><i>TOF-1</i> [P] 0 [P] 0 [P] 0 [P] 0 [P] 0 [P] 0 [P]</p> <p>Preset a delayed switching-off of 0-100 seconds for limit value 1.</p>
	<p>Back to menu group level, <i>RET</i>:</p> <p>With [P] the selection is confirmed and the device changes into menu group level „-AL1-“.</p>

The same applies for *-AL2-* to *-AL8-*.

Programming interlock, RUN:

Description see page 9, menu level *RUN*

6. Reset to default values

To return the unit to a **defined basic state**, a reset can be carried out to the default values.

The following procedure should be used:

- Switch off the power supply
- Press button **[P]**
- Switch on voltage supply and press **[P]**-button until „- - - - -“ appears in the display.

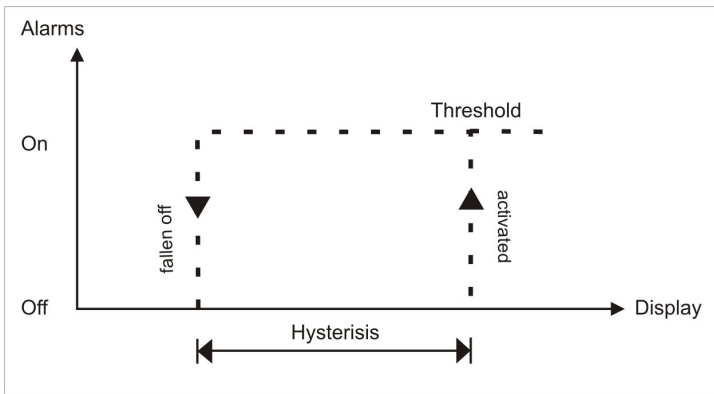
With reset, the default values of the program table are loaded and used for subsequent operation. This puts the device back to the state in which it was supplied.

Caution! All application-related data are lost.

7. Alarms / Relays

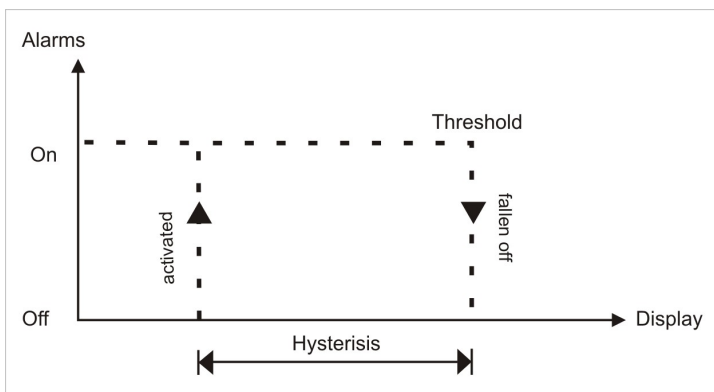
This device has 4 virtual alarms that can monitor one limit value in regard of an undercut or exceedance. Each alarm can be allocated to an optional relay output S1-S2; furthermore alarms can be controlled by events like e.g. Hold or min/max-value.

Function principle of alarms / relays	
Alarm / Relay x	Deactivated, instantaneous value, min/max-value, Hold-value
Switching threshold	Threshold / limit value of the change-over
Hysteresis	Broadness of the window between the switching thresholds
Working principle	Operating current / Quiescent current



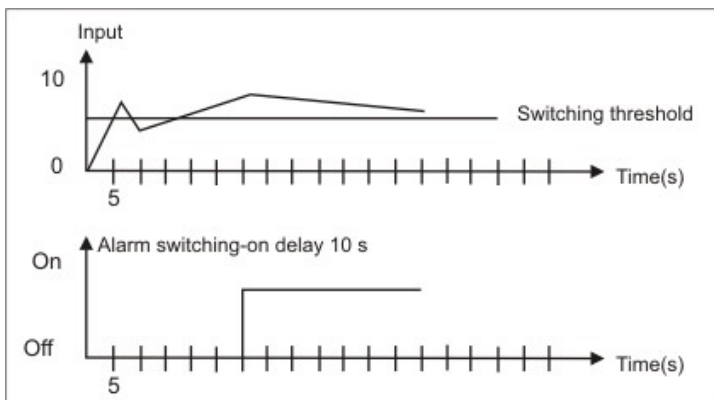
Operating current

By operating current the alarm S1-S2 is **off** below the threshold and **on** on reaching the threshold.



Quiescent current

By quiescent current the alarm S1-S2 is **on** below the threshold and switched **off** on reaching the threshold.



Switching-on delay

The switching-on delay is activated via an alarm and e.g. switched 10 seconds after reaching the switching threshold, a short-term exceedance of the switching value does not cause an alarm, respectively does not cause a switching operation of the relay. The switching-off delay operates in the same way, keeps the alarm / the relay switched longer for the parameterised time.

8. Technical data

Housing			
Dimensions	48x24x90 mm (BxHxD)		
	48x24x109 mm (BxHxD) incl. plug-in terminal		
Panel cut-out	45.0 ^{+0.6} x 22.2 ^{+0.3} mm		
Wall thickness	up to 3 mm		
Fixing	screw elements		
Material	PC Polycarbonate, black, UL94V-0		
Sealing material	EPDM, 65 Shore, black		
Protection class	standard IP65 (Front side), IP00 (Back side)		
Weight	approx. 200 g		
Connection	plug-in terminal; wire cross section up to 2.5 mm ²		
Display			
Digit height	10 mm		
Segment colour	red (optional green, yellow or blue)		
Range of display	-19999 to 99999		
Setpoints	one LED per setpoint		
Overflow	horizontal bars at the top		
Underflow	horizontal bars at the bottom		
Display time	0.1 to 10.0 seconds		
Input	Measuring range	Measuring error	Digit
Type L (Fe-CuNi old Type)	-200.0...-900.0°C	2 K	±1
Type J (Fe-CuNi)	-210.0...1200.0°C	2 K	±1
Type K (NiCr-NiAL)	-270.0...1372.0°C	2 K	±1
Type B (Pt30Rh-Pt6Rh)	80.0...1820.0°C	2 K	±1
Type S (Pt10Rh-Pt)	-50.0...1768.0°C	2 K	±1
Type N (NiCrSi-NiSi)	-270.0...1300°C	2 K	±1
Type E (NiCr-CuNi)	-270.0...1000.0°C	2 K	±1
Type T (Cu-Cu-Ni)	-270.0...400.0°C	2 K	±1
Type R (Pt13Rh-Pt)	-50.0...1768.0°C	2 K	±1
Digital input	< 2.4 V OFF, 10 V ON, max. 30 VDC R ₁ ~ 5 kΩ		

Accuracy	
Characteristic line error	< ± 1
Reference junction	semiconductor sensor
Temperature drift	100 ppm / K
Measuring time	0.1...10.0 seconds
Measuring principle	U/F-converter
Resolution	0.1°C or 0.1°F
Output	
Analog output	0/4-20 mA / burden $\leq 500 \Omega$; 0-10 VDC / burden $\geq 10 \text{ k}\Omega$, 16 bit
Switching outputs	2 PhotoMos (Closer)
Power pack	100-240 VAC 50/60 Hz / DC $\pm 10\%$ (max. 5 VA) 24 VDC $\pm 10\%$ galv. isolated (max. 4 VA)
Memory	
	EEPROM
Data life	≥ 100 years at 25°C
Ambient conditions	
Working temperature	0...50°C
Storing temperature	-20...80°C
Weathering resistance	relative humidity 0-80% on years average without dew
EMV	
	EN 61326
CE-sign	
	Conformity to directive 2014/30/EU
Safety standard	
	According to low voltage directive 2014/35/EU EN 61010; EN 60664-1

9. Safety advices

Please read the following safety advices and the assembly in *chapter 1* before installation and keep it for future reference.

Proper use

The **M3-7T-device** is designed for the evaluation and display of sensor signals.



Danger! Careless use or improper operation can result in personal injury and/or can damage the equipment.

Control of the device

The panel meters are checked before dispatch and sent out in perfect condition. Should there be any visible damage, we recommend close examination of the packaging. Please inform the supplier immediately of any damage.



Installation

The **M3-7T-device** must be installed by a suitably **qualified specialist** (e.g. with a qualification in industrial electronics).

Notes on installation

- There must be no magnetic or electric fields in the vicinity of the device, e.g. due to transformers, mobile phones or electrostatic discharge.
- **The fuse rating of the supply voltage should not exceed a value of 0.5A N.B. fuse!**
- Do not install **inductive consumers** (relays, solenoid valves etc.) near the device and **suppress** any interference with the aid of RC spark extinguishing combinations or free-wheeling diodes.
- Keep input, output and supply lines separate from one another and do not lay them parallel with each other. Position “go” and “return lines” next to one another. Where possible use twisted pair. This way best measuring results can be received.
- Screen off and twist sensor lines. Do not lay current-carrying lines in the vicinity. Connect the **screening on one side** on a suitable potential equaliser (normally signal ground).
- The device is not suitable for installation in areas where there is a risk of explosion.
- Any electrical connection deviating from the connection diagram can endanger human life and/or can destroy the equipment.
- The terminal area of the device is part of the service. Here electrostatic discharge needs to be avoided. Attention! High voltages can cause dangerous body currents.
- Galvanic isolated potentials within one complex need to be placed on an appropriate point (normally earth or machines ground). So, a lower disturbance sensibility against impacted energy can be reached and dangerous potentials, that can occur on long lines or due to faulty wiring, can be avoided.

10. Error elimination

	Error description	Measures
1.	<p>The unit permanently indicates overflow.</p> 	<ul style="list-style-type: none"> • The input has a very high measurement, check the measuring circuit. • With a selected input with a low voltage signal, it is only connected on one side or the input is open. • Not all of the activated supporting points are parameterised. Check if the relevant parameters are adjusted correctly.
2.	<p>The unit permanently shows underflow.</p> 	<ul style="list-style-type: none"> • The input has a very low measurement, check the measuring circuit . • With a selected input with a low voltage signal, it is only connected on one side or the input is open. • Not all of the activated supporting points are parameterised. Check if the relevant parameters are adjusted correctly.
3.	<p>The word HELP lights up in the 7-segment display.</p>	<ul style="list-style-type: none"> • The unit has found an error in the configuration memory. Perform a reset on the default values and reconfigure the unit according to your application.
4.	<p>Program numbers for parameterising of the input are not accessible.</p>	<ul style="list-style-type: none"> • Programming lock is activated • Enter correct code
5.	<p>Err1 lights up in the 7-segment display</p>	<ul style="list-style-type: none"> • Please contact the manufacturer if errors of this kind occur.
6.	<p>The device does not react as expected.</p>	<ul style="list-style-type: none"> • If you are not sure if the device has been parameterised before, then follow the steps as written in <i>Chapter 6</i>. and set it back to its delivery status.